

Figure 1

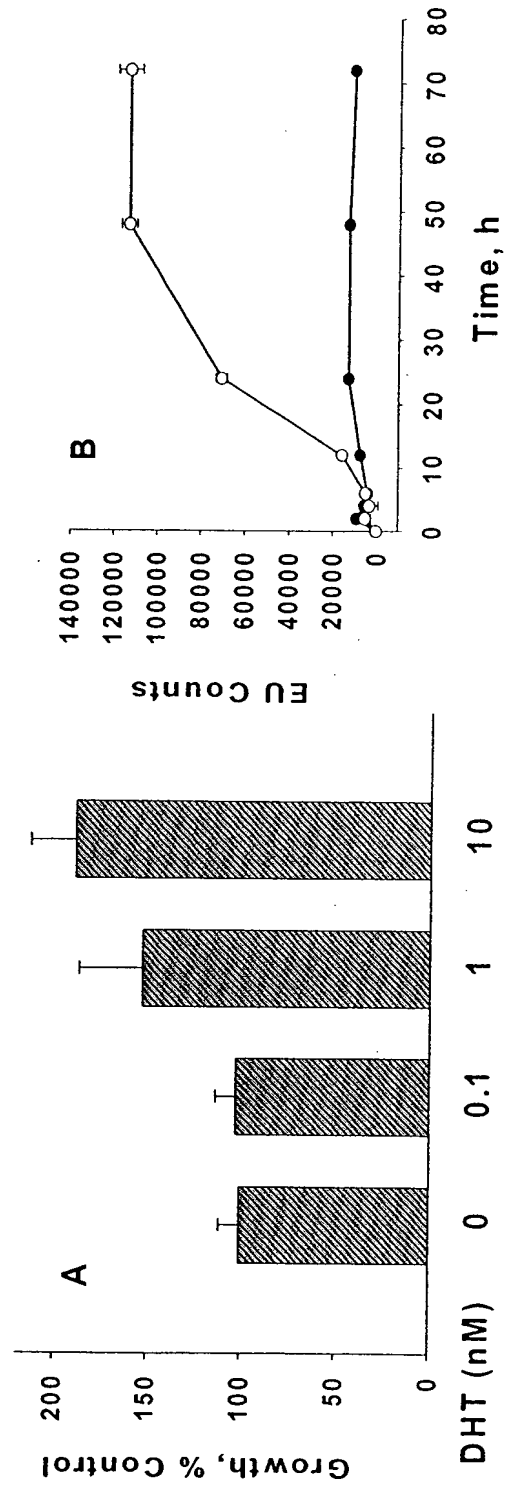


Figure 2

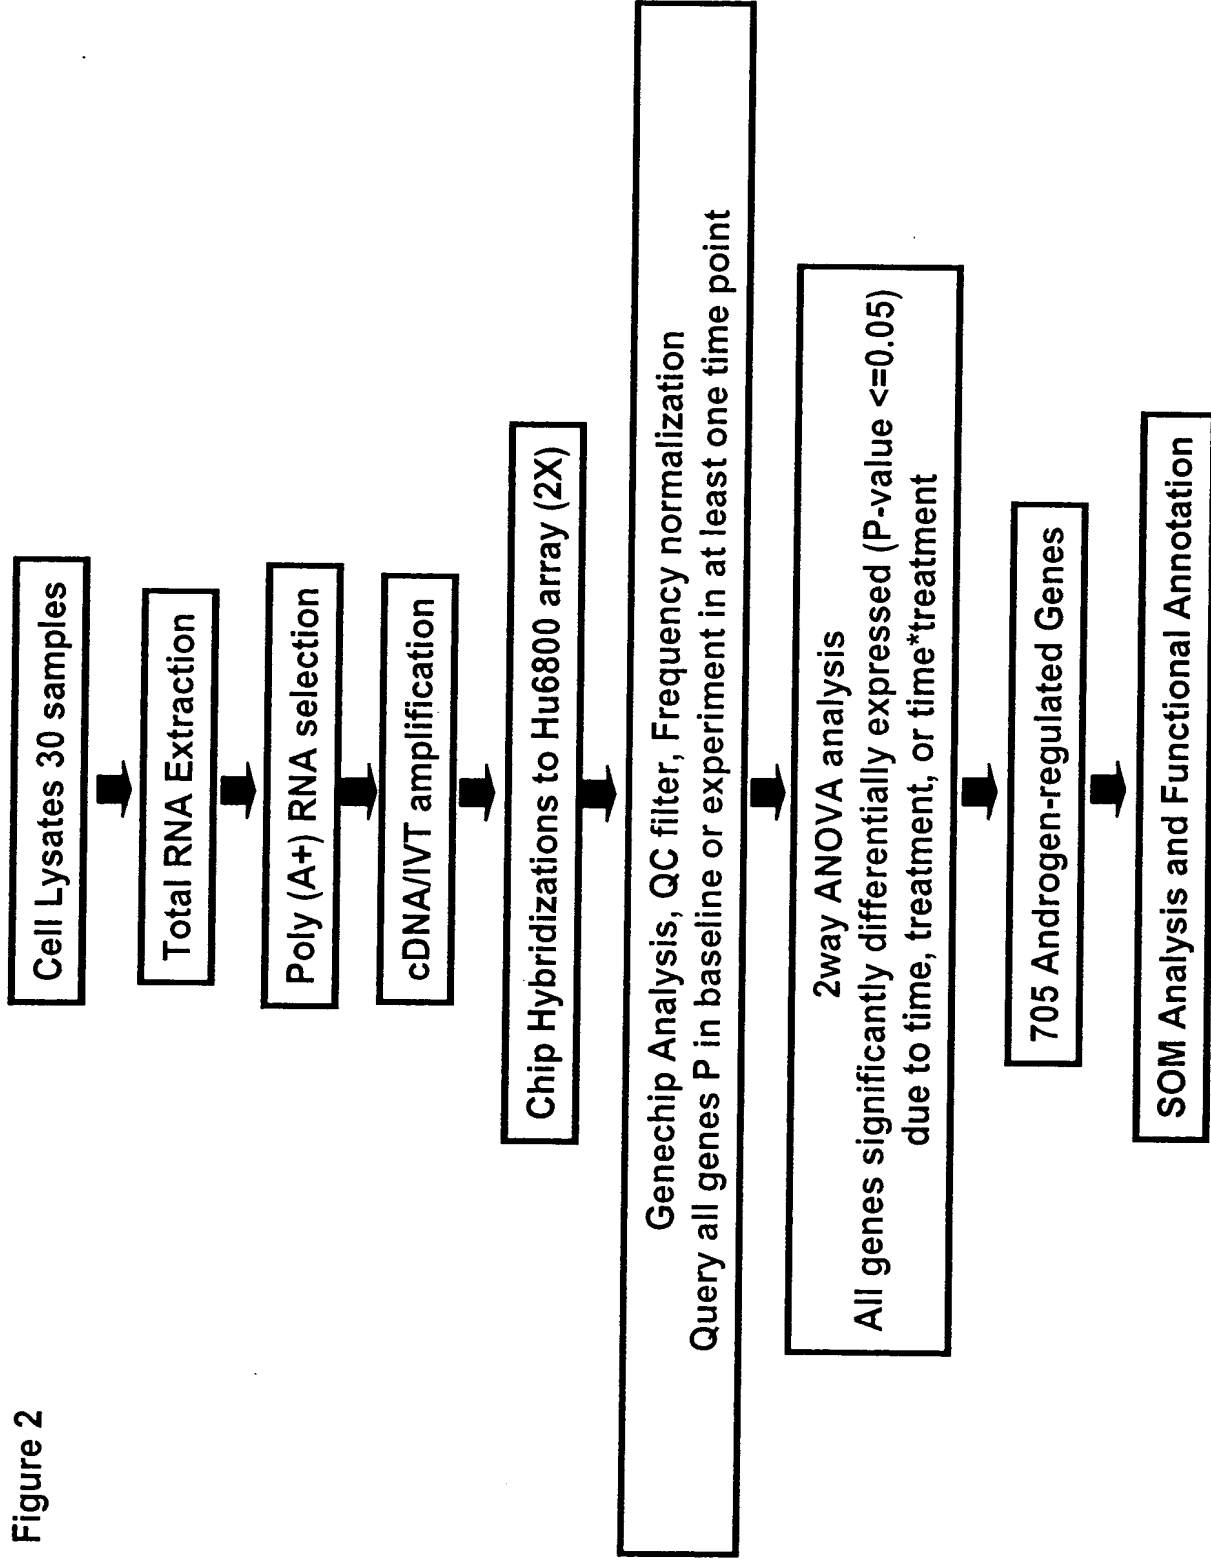


Figure 3

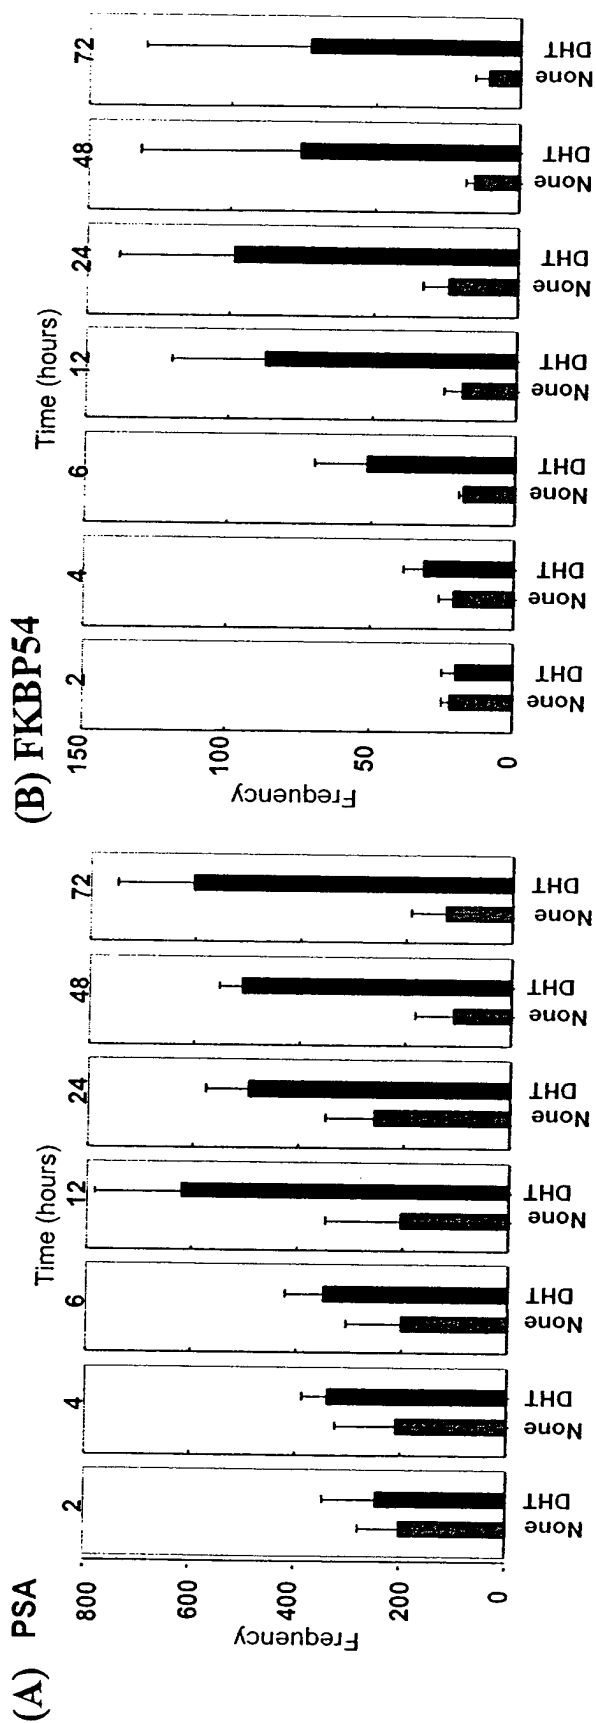


Figure 3 shows the frequency of PSA and FKBP54 over time (2, 4, 6, 12, 24, 48, 72 hours) for DHT and None groups. The y-axis represents Frequency (0-800 for PSA, 0-150 for FKBP54). The x-axis represents Time (hours). Error bars are shown for each data point.

Figure 4

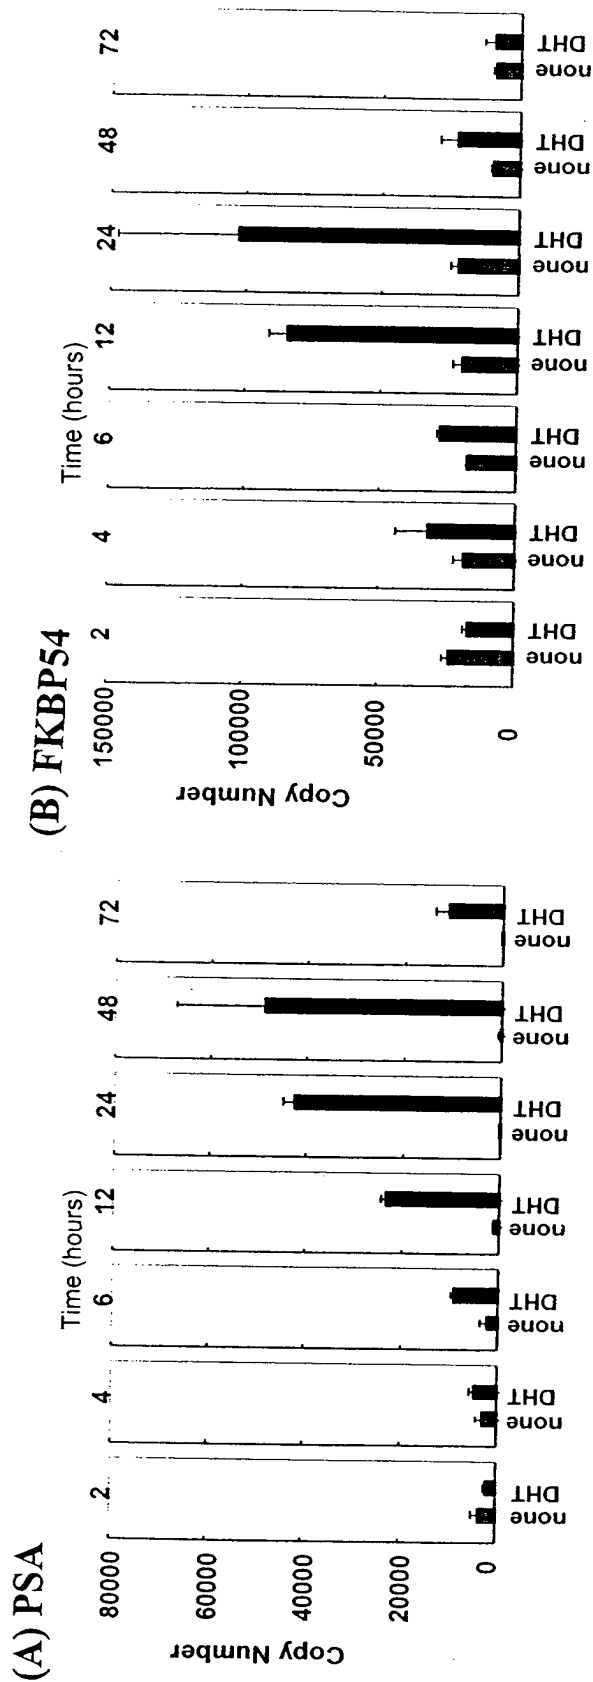


Figure 5

